

agappe

BIOLIS30i

Automated Clinical Chemistry Analyzer



JAPAN QUALITY



TOKYO BOEKI MEDISYS

LABORATORY SOLUTION



Improved user-friendly interface and test efficiency

The latest model of TMS series meeting various needs of clinical laboratory tests

***HbA1c Measurement Directly
from Whole Blood***



Compact & Easy Operability & Excellent Function



Brand new user interface

- Intuitive screen layout with a sense of unity
- Item parameter in one screen relieving the bother of page feeding

Upgraded operability

- Various touch panel operation (swipe-to-select / drag & drop) contributing to better facility of operation
- Enlarged buttons for reducing operation errors

Upgraded throughput

- 270 tests/hour (maximum 450 tests/hour with ISE)

Auto hemolysis of whole blood sample for HbA1c

- Automatic process on board contributing to the test efficiency and accuracy

Automatic sample clot detection

- Automatic detection & clean-up of sample probe clots (such as !brin)

Crash prevention

- Prevent reagent & sample probes from crash during operation for safety


Automatic startup and shutdown

- Stress-free operation by cutting waiting time

Ethernet connections

- Ethernet connections between machine and operation PC for higher-speed and more stable communication

Main unit arrangement

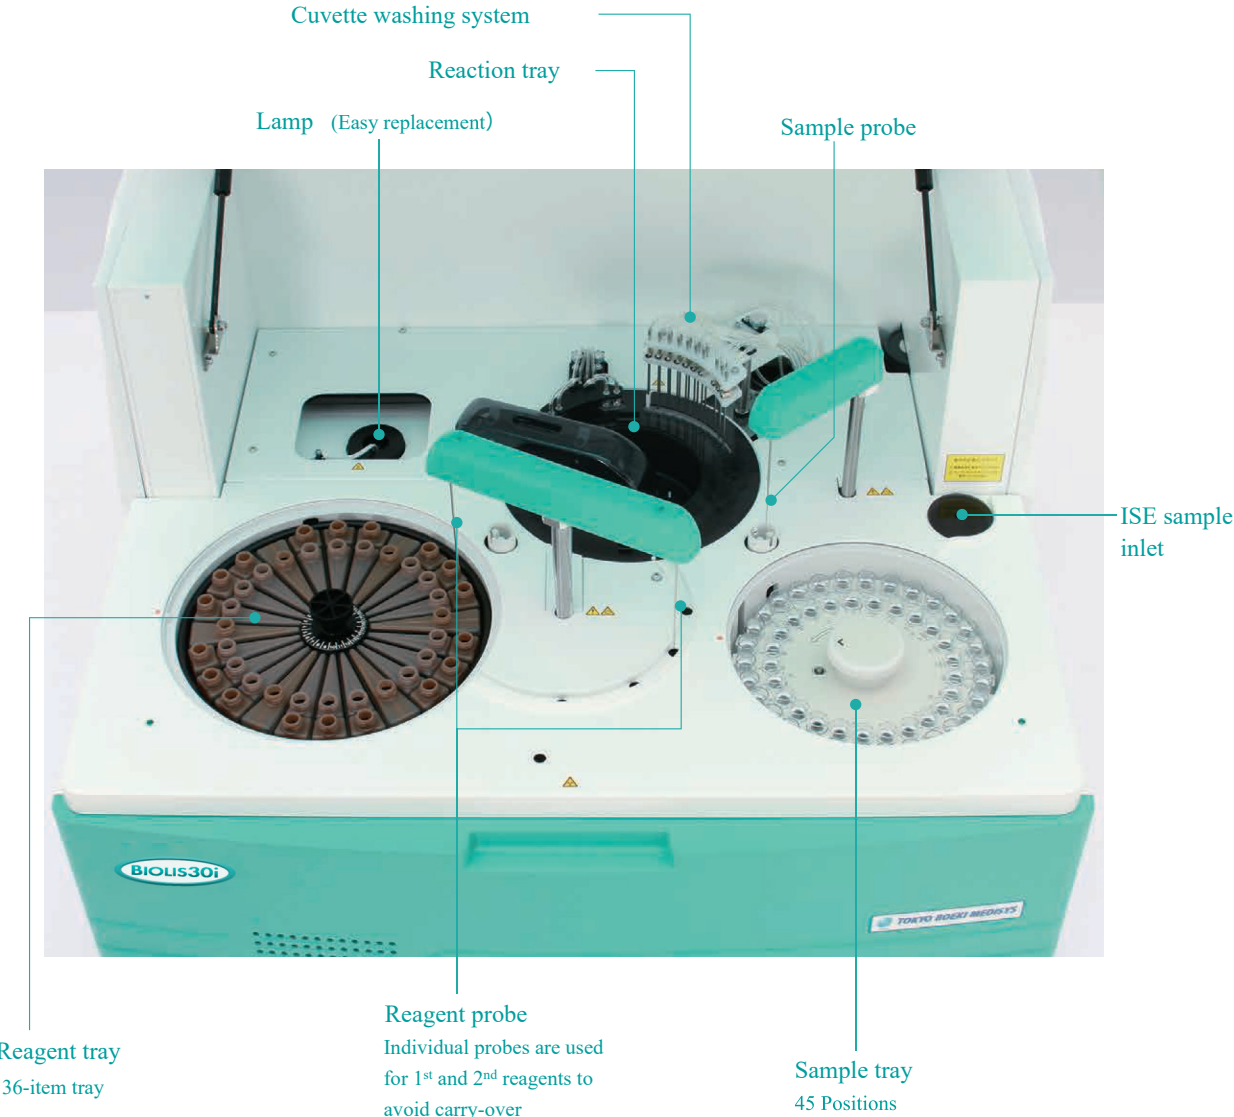

Specifications

Analysis	System	Discrete single line random access multi-test analysis
	Number of test items on board	36+3 (ISE)
	Throughput	270 tests/hour, 450 tests/hour including ISE, 90tests/hour for HbA1c only
	Analysis method	End point, Rate, ISE
Sample	Calibration curve	8 kinds (linear , spline, etc)
	Sample kind	Serum, Plasma, Blood cell, Urine, Dialysis, CSF (ISE not available for CSF and Blood cell)
	Sample container	Sample cups, primary tube (5, 7, 10ml)
	Number of samples on board	Software tray (30 positions for primary sample, and 45 positions for standard and blank sample)
	Sample tray mode (software tray)	Selectable modes for patient sample, calibration and QC
	Sample dispensing volume	2.0 ~ 25.0 μ L (0.1 μ L step)
	Dilution ratio	0.5 ~ 100 times
Reagent	STAT	Available during measurement (step between samples by priority)
	Reagent tray	36 items (removable)
	Number of bottles on board	72 (36 items)
	Bottle size	36 items : 13, 25, 40 ml 24 items : 20, 40, 60 ml
	Reagent dispensing volume	R1 : 140 ~ 300 μ L (1 μ L step) , R2 : 20 ~ 260 μ L (1 μ L step)
	Reagent storage	24 hours cooling
Reaction	Reagent volume check	Level sensing or count down
	Cuvette material	Plastics (semi-disposable)
	Reaction volume	140 ~ 400 μ L
	Reaction time	approx 10 min. (1st reaction 5 min., 2nd reaction 5min.)
	Reaction temperature	37 $\pm$ 0.1 $^{\circ}$ C
	Optical measurements	Fixed 13 wavelengths (340 ~ 800 nm)
	Optical source	Tungsten halogen lamp
	Optical range	OD 0.0 ~ 2.5
	Cuvette washing	Auto washing with heated water and 2 kinds of washing solutions
Interface	Reaction waste collection	Reaction waste stored in a dedicated tank
	Pure water consumption	Maximum 3.8 L/hour
	Operation	Personal computer
	OS	Windows 10
	Reaction monitor	Optical absorbance graphic display
Option	Quality control	Current, Daily and Cumulative QC. Westgard algorithms
	Output	Ethernet connection
Option	ISE module	
	Sample barcode reader, Reagent barcode reader	


Specifications are subject to change without notice .

Installation

Conditions

Item	Description
Dimensions and Weight	Analyzer W800 × D670 × H555 (mm) Approx. 95Kg
Power supply	AC 100/115/220/230V、 50/60Hz Voltage fluctuation less than 10%
Power consumption	600VA
Grounding	Earth resistance of ground terminal should be less than 100 Ω
Ambient temperature	15~30 $^{\circ}$ C
Humidity	45~85% (No condensation)
Water consumption	Max 3.8 l / hour
Waste liquid	Separate drainage (low and high density waste)

The space required for installation

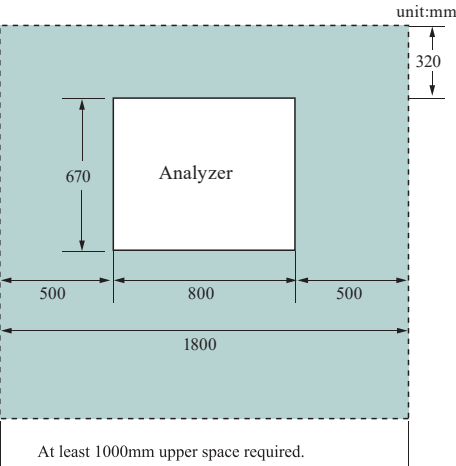


Test Items List

Clinical chemistry	LD(LDH)	AST(GOT)	ALT(GPT)	ALP	γ -GTP	CK(CPK)	CK-MB
	ChE	AMY	P-AMY*	LAP	CRE	UA	BUN
	Cys-C	TG	T-CHO	HDL-C	LDL-C	TP	ALB
	IP	Mg	Ca	Fe	TIBC	Zn	Cu
	GLU	HbA1c	1,5-AG*	GA*	μ TP	μ ALB	IRI
	L-FABP*	T-BIL	D-BIL	TTT*	ZTT*	NH3*	NEFA*
	PL *	SIA *	Fer				
Couglution*	AT	FDP	D-dimer				
Immuno-assay	CRP	RF	TPAb*	RPR *	IgG	IgA	IgM
	IgE	MMP-3*					
TDM*	VCM	ABK	TPM	MTX	EVER	TACR	BRP
	CBZ	DIG	HAL	PB	PHT	THEO	VPA
ISE	Na	K	Cl				

* Above includes test items under verification.


User Interface

Run monitor screen

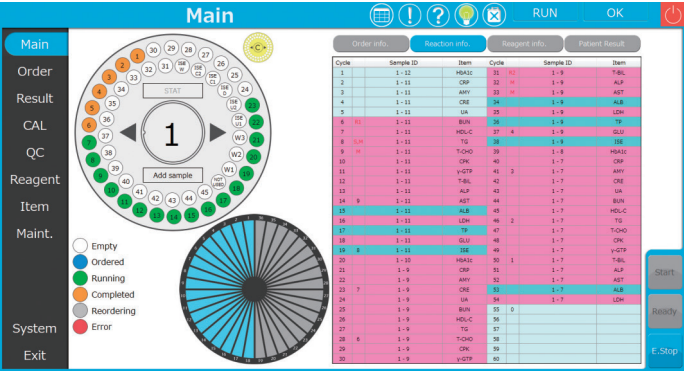


Monitor measurement info by cycles

Journal screen

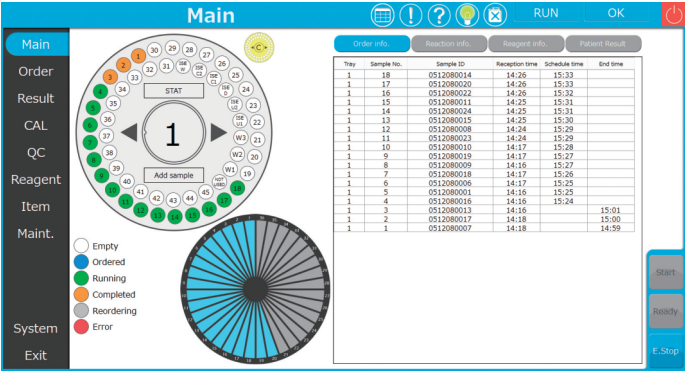


View sample ordered time and result out-put time

Order screen

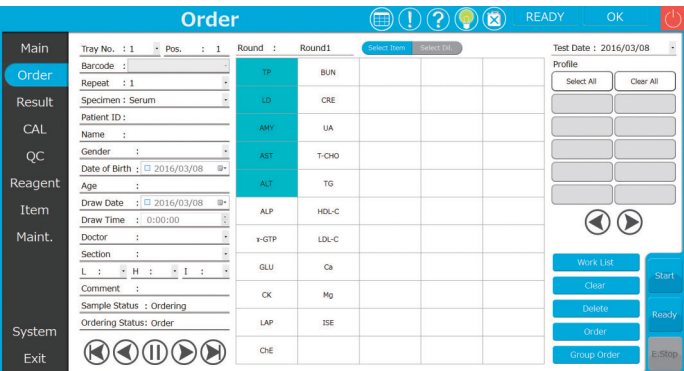


Easy to select test items by swiping the touch screen

QC graph screen

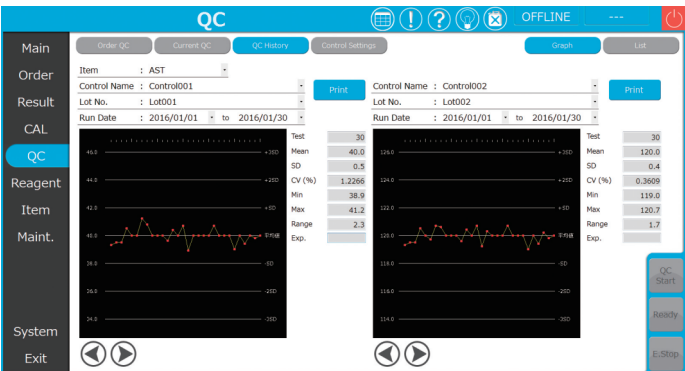


Current,daily,and cumulative QC

Auto startup & shutdown screen

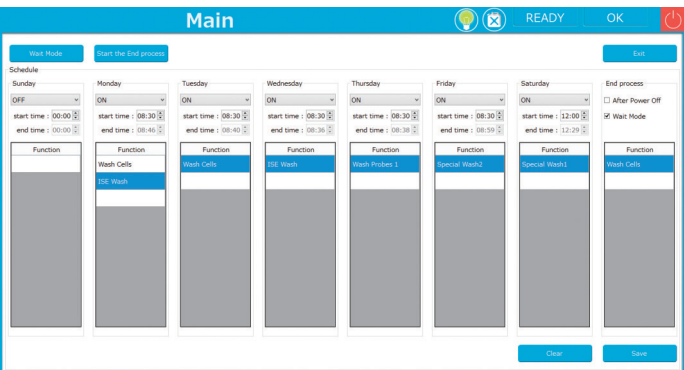

Auto maintenance available before shutdown


Result screen

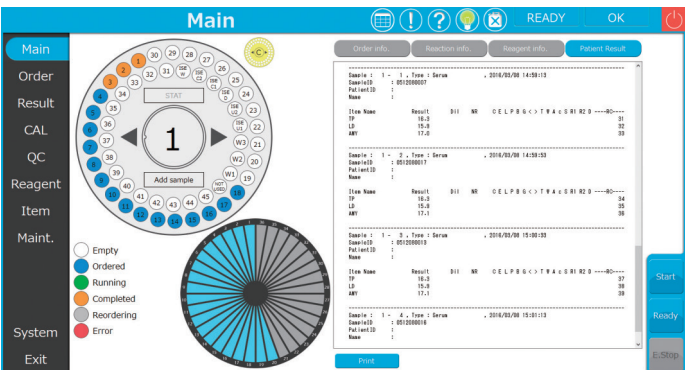

Show current day test results
(Separate printer needed for output)

Air pressure mixing system

Our original system for mixing the sample and reagent using air pressure alone.

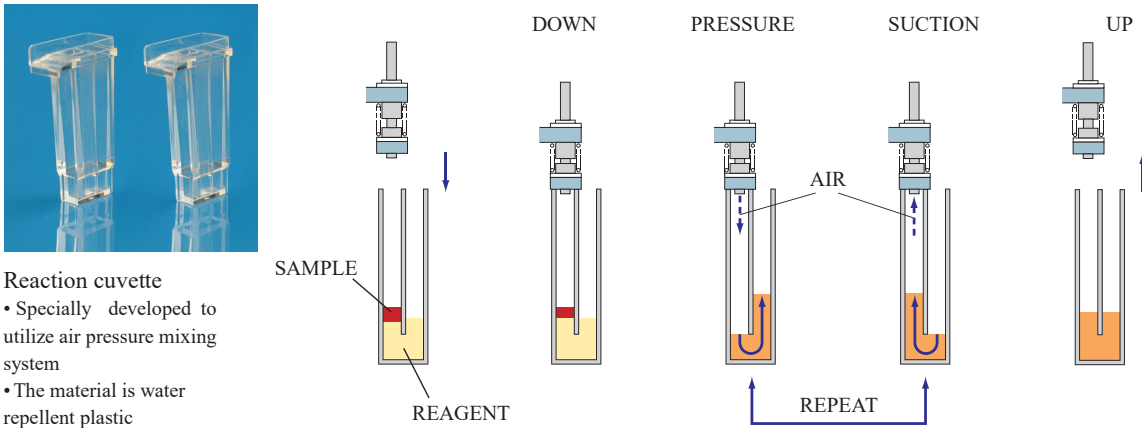


Reaction cuvette
• Specially developed to utilize air pressure mixing system
• The material is water repellent plastic (Semi-disposable)


Advantages of Air Pressure Mixing

- No carry-over because a stirrer is not used
- No water consumption for stirrer washing
- No dilution of the reaction solution by washing water from the stirrer

HbA1c sample preparation and measurement

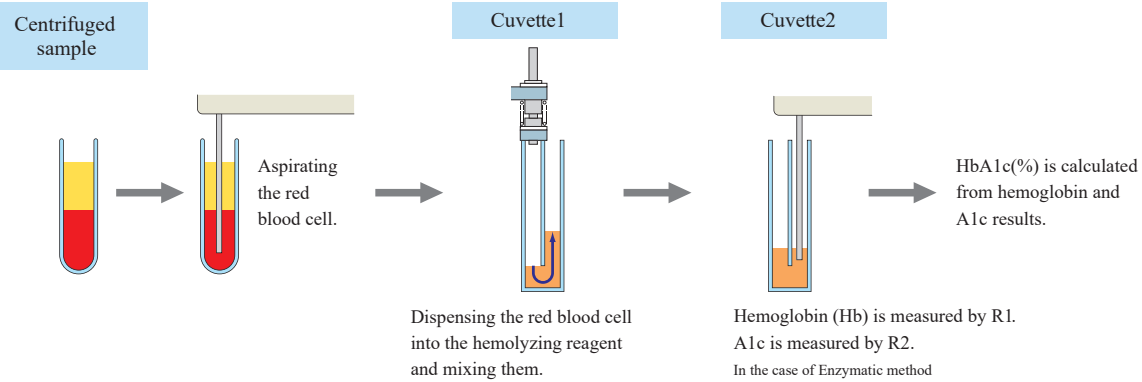

ISE module (OPTION)

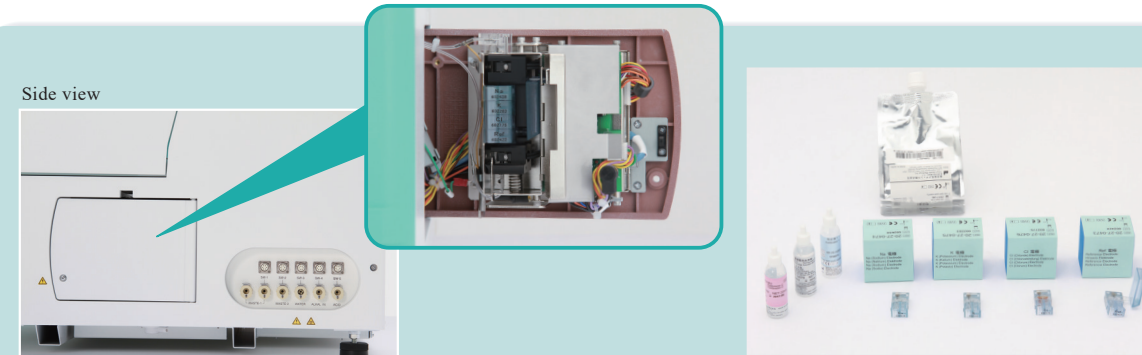

ISE is Direct Method

- Throughput is 450 tests/hour including ISE
- ISE module is equipped with Biolis 30i
- Easy to replace electrodes

Consumables for ISE module

- Calibrators
- Cleaning solution
- Electrode (Na, K, Cl, Ref)



TOKYO BOEKI MEDISYS INC.

Headquarters & R&D Center

1-14-21, Higashitoyoda, Hino, Tokyo, 191-0052 Japan

Tel: +81-42-587-7777 Fax: +81-42-587-7781

URL <http://www.tb-medisys.co.jp/english/>

Marketed by,

AGAPPE DIAGNOSTICS LIMITED, "Agappe Hills", Pattimattom (PO), Dist.

Ernakulam, Kerala - 683 562, India.

TEL: + 91 484 2867000 | FAX: +91 484 2867222 | agappe@agappe.in | www.agappe.com



EN ISO 13485 : 2016