

Technical Specifications

Method	Time-Resolved Fluorescence Immunoassay (TRFIA)
Specimen	Serum/Plasma / Whole Blood
Weight	1.3 kg
Dimensions	225mm×152mm×105mm (L×W×H)
Screen	7 inch touch screen
Data Storage	10000 Nos.
Printer	Built-in thermal printer
Battery	Built-in lithium battery (standby time: 6 hrs)
Power Source	AC100V – 240V AC, 50-60Hz, 60VA
Communication	RS232 (LIS/HIS), USB

► **Test Items:**

Pack Size - 25 Tests

Category	Test Item	Specimen Type	Sample Volume	Reaction Time	Measuring Range
Cardiac	cTnI	S	100µl	10min	0.05 -40ng/mL
	cTnI/CK-MB/Myo	S	100µl	10min	cTnI:0.05-40ng/mL
					CK-MB:0.2 -80ng/mL
					Myo:20 -500ng/mL
	NT-proBNP	S	100µl	15min	50-25000pg/mL
Thyroid	D-Dimer	P	100µl	10min	0.1-10 µg/mL
	T3	S	100µl	15min	0.5-10nmol/mL
	T4	S	100µl	10min	10-350nmol/mL
	TSH	S	100µl	15min	0.1-60µ IU/mL
Bone Metabolism	25OH-VITD	S	5µl	10min	5.0-70ng/mL
Tumor Marker	PSA	S	100µl	10min	0.1-100ng/mL
Fertility	ß-HCG	S	100µl	15min	2.0-20000mIU/mL
	AMH	S	100µl	10min	0.1-50ng/mL
	LH	S	100µl	10min	1.02-200mIU/mL
	FSH	S	100µl	10min	1-200mIU/mL
	PRL	S	100µl	15min	200-4000µ IU/mL
	Progesterone	S	100µl	10min	0.8-50ng/mL
Inflammation	PCT	S	100µl	10min	0.1-50ng/mL
	IL-6	S	100µl	15min	5-2000pg/mL
Iron Metabolism	Ferritin	S	5µl	15min	10-1000 ng/ml

S* stands for Serum and P* stands for Plasma

EN ISO 13485 : 2016



Toll Free No: 1800 425 7151


AGAPPE DIAGNOSTICS LTD.

“Agappe Hills”, Pattimattom (PO), Dist. Ernakulam, Kerala - 683 562, India.
TEL: + 91 484 2867000 | productcorp@agappe.in | www.agappe.com



**Quantitative | Sensitive
Rapid | Reliable**

**Thyroid | Cardiac | Fertility
Inflammation | Bone Metabolism**

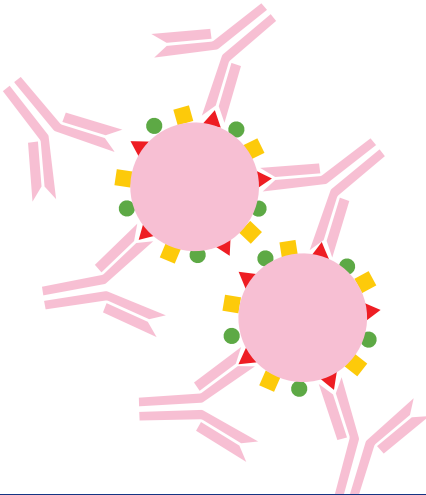



Mispa Revo Plus

Dry Fluorescence Immunoassay Analyzer
(Time Resolved Fluorescence Immunoassay method - TRFIA)

YOUR BEST PARTNER IN DIAGNOSTICS

ADL/BR/REVO+/R04-01/26 Company reserves the right to change any design and technical features of the product at any time, if needed.

Mispa Revo Plus uses the advanced method of Time-Resolved Fluorescence Immunoassay (TRFIA), for the in-vitro quantitative detection of bio-markers for cardiovascular diseases, fertility hormones, thyroid function, bone metabolism, inflammation and other diseases.




ACCURATE RESULTS
ANYTIME & ANYWHERE


TIME-RESOLVED FLUORESCENCE IMMUNOASSAY (TRFIA) METHOD:

TRFIA Is Super-Sensitive Detection Technique characterized by Specific fluorescence of Rare Earth Ions (eu^{3+}).

- Y Highly Sensitive ▶ Overcomes Instability of Enzyme Marker.
- Y High Fluorescence Intensity.
- Y Specific Emission Spectrum of $615 \pm 5 \text{ nm}$.
- Y Long Fluorescence Lifetime $714 \mu\text{s}$.
- Y Large Stokes Displacement.
- Y Distinguish Specific Fluorescence from Non-specific Fluorescence by Wavelength Resolution.

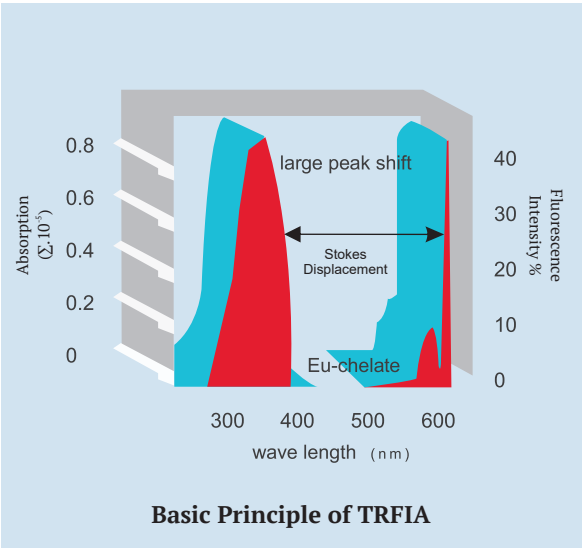


► Easy Operation:

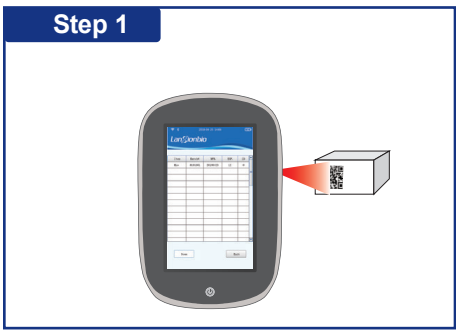

QR Code Calibration



Information Input

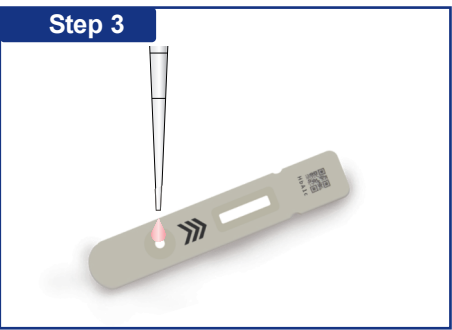

Dispense Sample



Press 'Test' to start Testing



Automatic Detection



Result Output

SMALL | COMPACT | PORTABLE

QUICK | RELIABLE | ACCURATE